


Add/Remove Analytes

Add Analytes

- Expand the "Analytes Not Being Tested" panel by clicking on the icon .
- Select all the analytes that are now being tested in your laboratory and use the same instrument. Click on the "Test Selected Analytes" button.

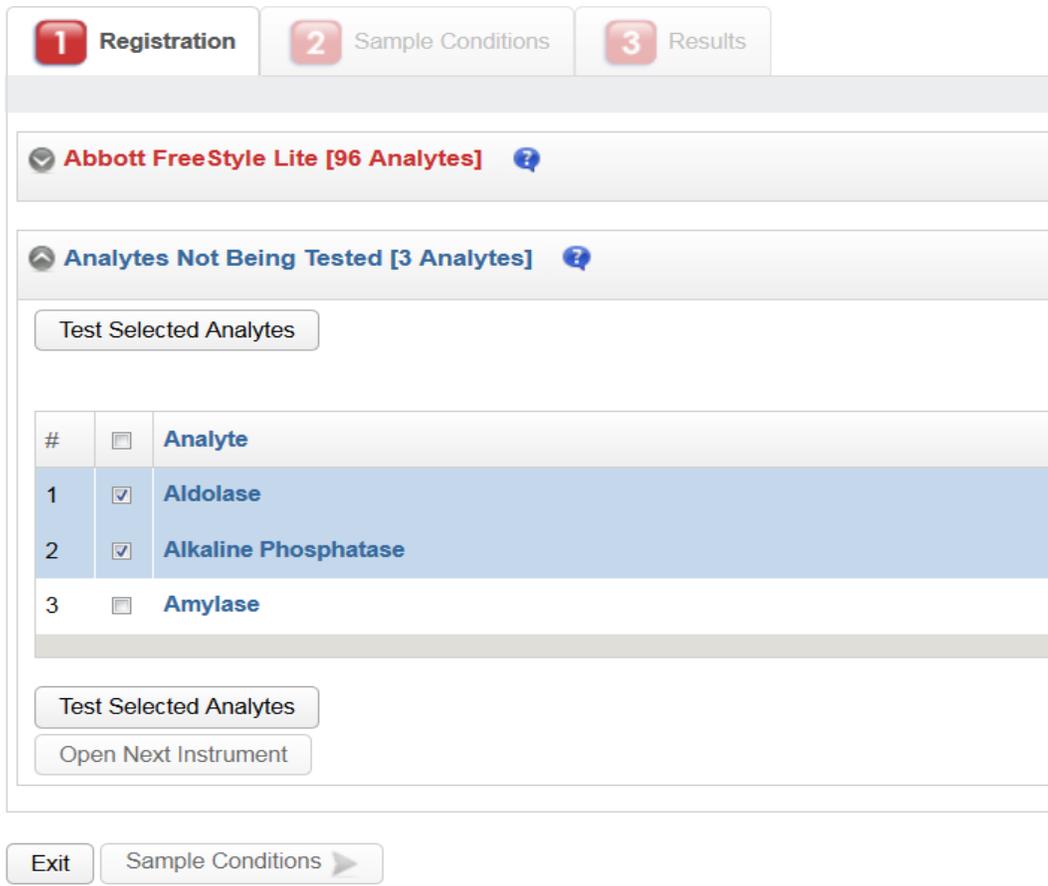

1 Registration 2 Sample Conditions 3 Results

Abbott FreeStyle Lite [96 Analytes] ?

^ Analytes Not Being Tested [3 Analytes] ?

Test Selected Analytes


#	<input type="checkbox"/>	Analyte
1	<input checked="" type="checkbox"/>	Aldolase
2	<input checked="" type="checkbox"/>	Alkaline Phosphatase
3	<input type="checkbox"/>	Amylase

Test Selected Analytes


Open Next Instrument

Exit Sample Conditions ▶

- Add a new instrument by selecting the Manufacturer and Instrument Model under "Register New Instrument". Add a Nickname and a Serial Number (Optional) and click on "Add & Select".
Or add an existing instrument by selecting your instrument under "Instrument Currently Registered for This Subscription" or under "Other Instruments".

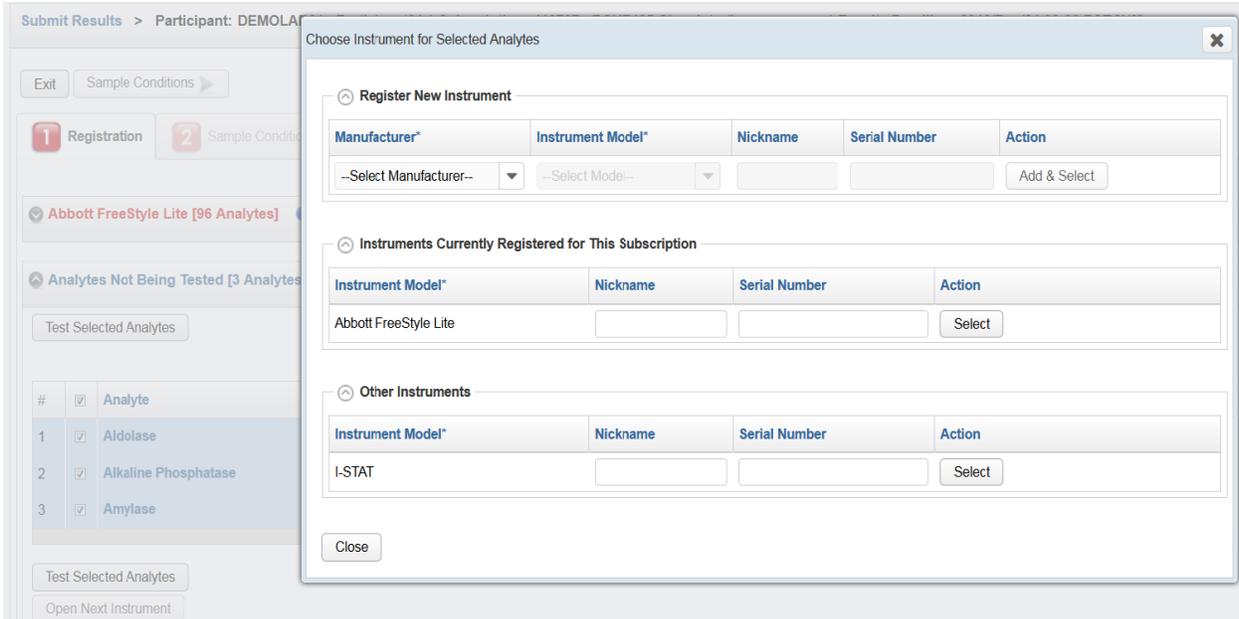

- d. The analytes will be moved to the corresponding Instrument panel, where you can choose the reagent manufacturer, the reagent catalog number and the reagent submethod.

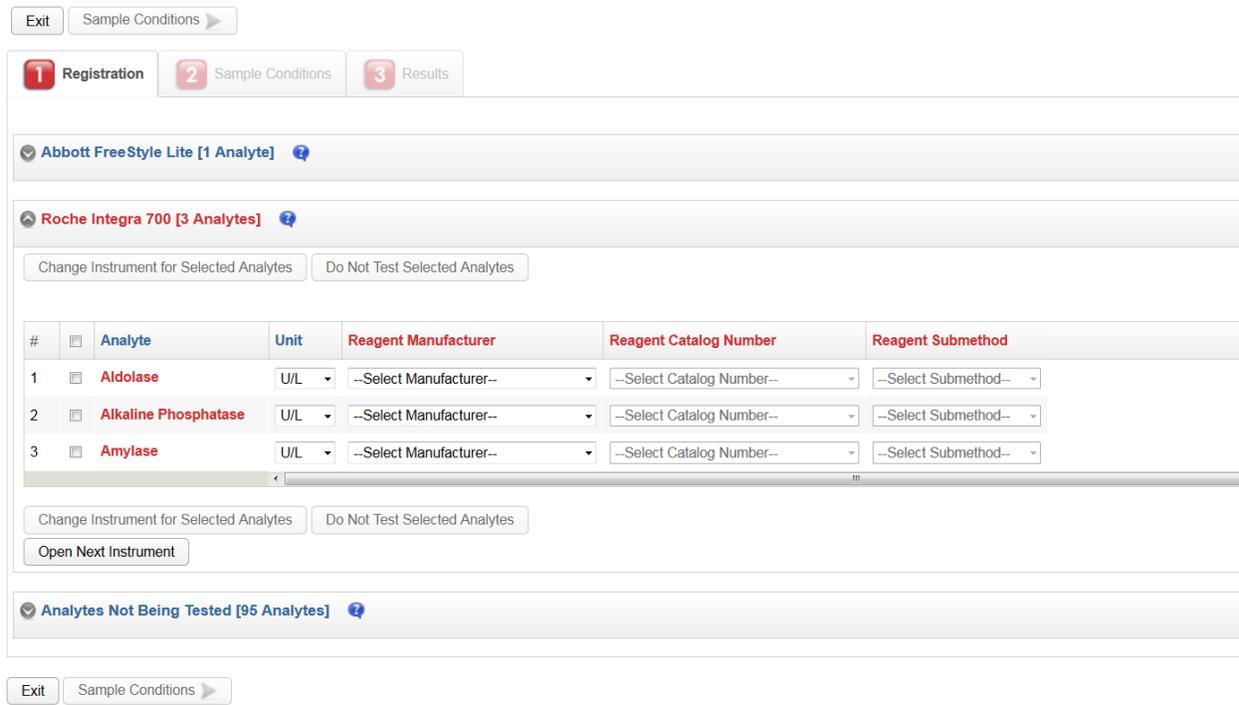

Repeat steps b. to d. until all the analytes that are now being tested have been added and associated with instruments.

Remove Analytes

a. Select the analyte you would like to remove by clicking the check box.

Exit Sample Conditions ▶

1 Registration 2 Sample Conditions 3 Results

Abbott FreeStyle Lite [5 Analytes] ?

Change Instrument for Selected Analytes Do Not Test Selected Analytes

Show Analytes: 1.5

#	<input type="checkbox"/>	Analyte	Unit	Reagent Manufacturer	Reagent Catalog Number	Reagent Submethod
1	<input checked="" type="checkbox"/>	Alanine Aminotransferase	U/L	--Select Manufacturer--	--Select Catalog Number--	--Select Submethod--
2	<input type="checkbox"/>	Albumin	g/L	Amresco Inc.	Amresco CAT# 1032500	Bromocresol Green
3	<input checked="" type="checkbox"/>	Bilirubin - Direct	µmol/L	--Select Manufacturer--	--Select Catalog Number--	--Select Submethod--
4	<input checked="" type="checkbox"/>	Bilirubin - Total	µmol/L	--Select Manufacturer--	--Select Catalog Number--	--Select Submethod--
5	<input checked="" type="checkbox"/>	Calcium, ionized	mmol/L	--Select Manufacturer--	--Select Catalog Number--	--Select Submethod--

Show Analytes: 1.5

Change Instrument for Selected Analytes Do Not Test Selected Analytes

Open Next Instrument

b. Once all the analytes that are not being tested are selected click "Do Not Test Selected Analytes". This will remove the analytes from the list and store them in the "Analytes Not Being Tested" panel.